ANALIZA BIAŁEK

Scan for verify

100015622

Laboratory of Analysis

Client: Peplabs
Order number: 100015622
Name: PEPLABS SEMAX
Number of samples: 1 vial

Batch number: ------
Receive date: 2026-06-23
Start date: 2026-06-26
End date: 2026-07-01

Sample identification

Substance	Method of taking a sample	Form
Semax	Sample provided by customer	White powder in a glass vial


Results

Substance	Sample name	Content	Purity
Semax	PEPLABS SEMAX 10MG	10,22mg	99%
Endotoxin Level	PEPLABS SEMAX 10MG	5,52EU/vial	------

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 10,22mg. Height the measurement error is +-0,05mg.

Chromatogram

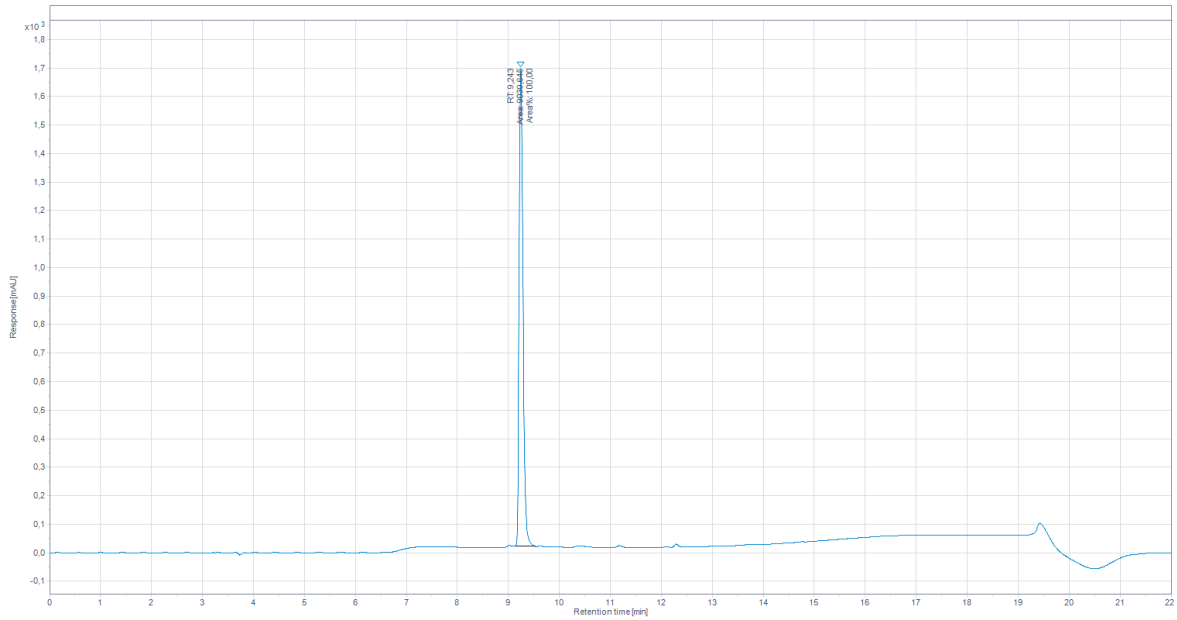

Password

I6J3LMXZ

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

Scan for verify

100015622

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

I6J3LMXZ

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając